




Transducer Certificate of Conformity
Compliant to ASTM E-1065


Date 10/18/2018
Part Number 113-144-280

Serial Number S000038
Description FIP---XDCR ISS 5X.5 APHSF

Real Time Waveform

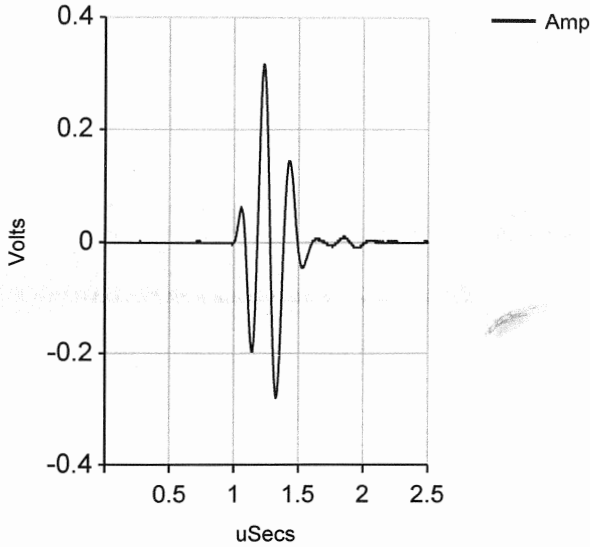

Frequency Spectrum

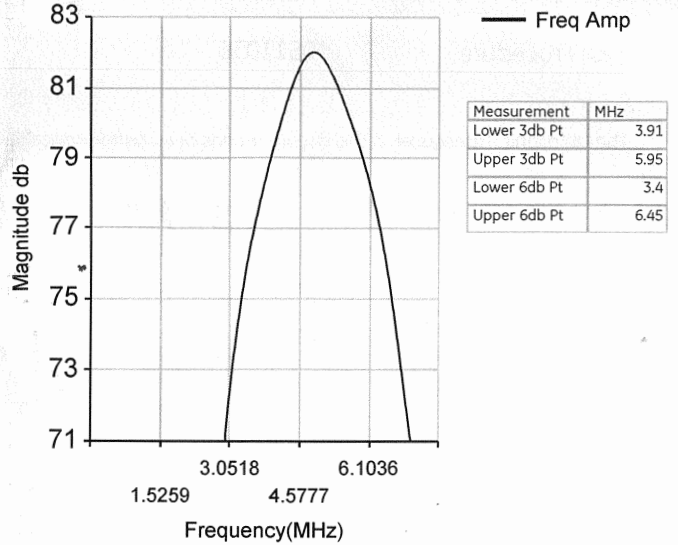

Waveform is first return echo from indicated target.

Test Data

UTA	Setting
Receiver Imp	50
Pulser Imp	LOW
Energy	LOW
Voltage	100
Mode	T/R
Pulser	UTA
HP Filter	1.0 MHz
LP Filter	10 MHz
Target	1.0 " 303 STEEL @ 3 0" W.P.
UTA Gain	1.6

Test	Min	Measured	Max
Loop Sensitivity(db)	-51	-40.29	-37
Center Freq(MHz)	4	4.93	6
Peak Freq(MHz)	4.5	4.85	5.5
6db Bandwidth %	50	61	
20db Ringdown(usec)		0.53	0.75
Focus(in)		2.52	

UTA SN DA0518
UTA Cal Due Date 01/16/2019
O-Scope SN C048089
O-Scope Cal Date 01/16/2019

Target SN



Transducer Certificate of Conformity
Compliant to ASTM E-1065

Date	10/18/2018	Serial Number	S000038
Part Number	113-144-280	Description	FIP---XDCR ISS 5X.5 APHSF
Inspector	MM		
Software	FNT0040	Rev	H
Test Procedure	0511036		

The Ultrasonic Transducer in this document has been performance tested and meets all manufacturing specifications.

The accuracy of the transducer described above has been confirmed by factory standard test equipment and laboratory reference standards traceable to the National Institute of Standards and Technology. This facility's Quality System is registered to ISO 9001-2008 and is compliant to MIL-STD-45662A and ANSINCSL Z540-1-1994.

GE Inspection Technologies, LP
50 Industrial Park Rd.
Lewistown, PA 17044

Tel: 717.242.0327
Fax: 717.242.2606
GEInspectionTechnologies.com