




Transducer Certificate of Conformity
Compliant to ASTM E-1065


Date 03/11/2019
Part Number 113-145-591

Serial Number S000012
Description FABP--MSWQC-ALP 7.5X.5

Real Time Waveform

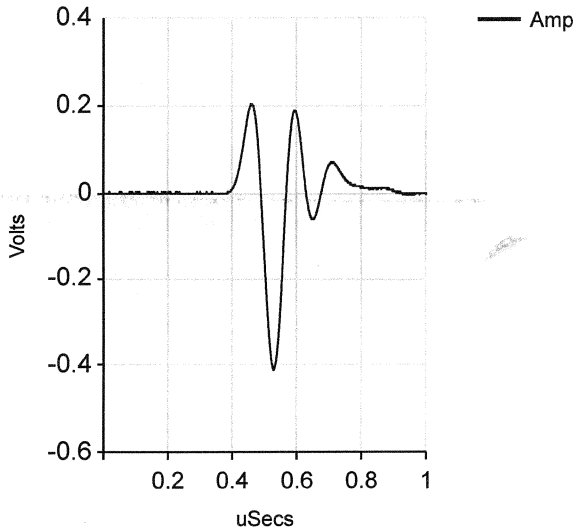

Frequency Spectrum

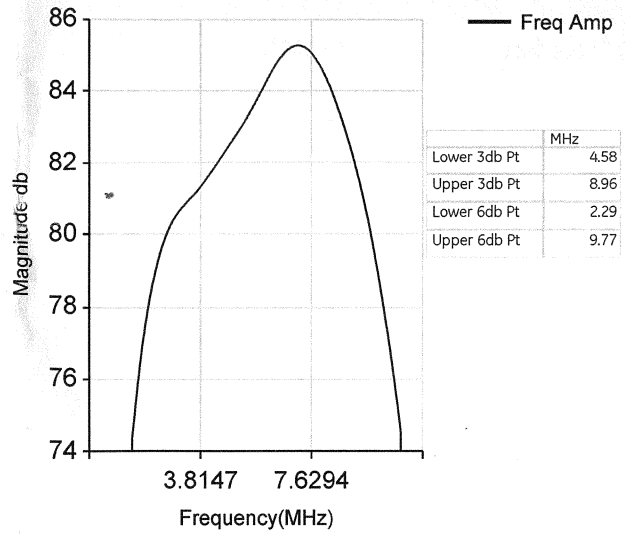

Waveform is first return echo from indicated target.

UTA	Setting
Receiver Imp	50
Pulser Imp	LOW
Energy	MID-HIGH
Voltage	100
Mode	T/R
Pulser	UTA
HP Filter	1.0 MHz
LP Filter	22.5 MHz
Target	0.25 Plexi Glass

Test Data

Test	Min	Measured	Max
Loop Sensitivity(db)	-52	-46.05	-46
Center Freq(MHz)		6.03	
Peak Freq(MHz)	6.75	7.13	8.25
6db Bandwidth %		124	
20db Ringdown(usec)		0.324	0.38

UTA SN DF0517
UTA Cal Due Date 07/01/2021
O-Scope SN C048089
O-Scope Cal Date 01/25/2020

Target SN

UTA Gain 6.1



Transducer Certificate of Conformity
Compliant to ASTM E-1065

Date	03/11/2019	Serial Number	S000012
Part Number	113-145-591	Description	FABP--MSWQC-ALP 7.5X.5
Inspector	MD		
Software	FNT0040	Rev	H
Test Procedure	0511416		

The Ultrasonic Transducer in this document has been performance tested and meets all manufacturing specifications.

The accuracy of the transducer described above has been confirmed by factory standard test equipment and laboratory reference standards traceable to the National Institute of Standards and Technology. This facility's Quality System is registered to ISO 9001-2008 and is compliant to MIL-STD-45662A and ANSINCSL Z540-1-1994.

GE Inspection Technologies, LP
50 Industrial Park Rd.
Lewistown, PA 17044

Tel.: 717.242.0327
Fax: 717.242.2606
GEInspectionTechnologies.com