




Transducer Certificate of Conformity  
Compliant to ASTM E-1065


Date 05/21/2018  
Part Number 113-223-590

Serial Number SAH0023  
Description FABP--MSWQC-GAM 3.5X.25

Real Time Waveform

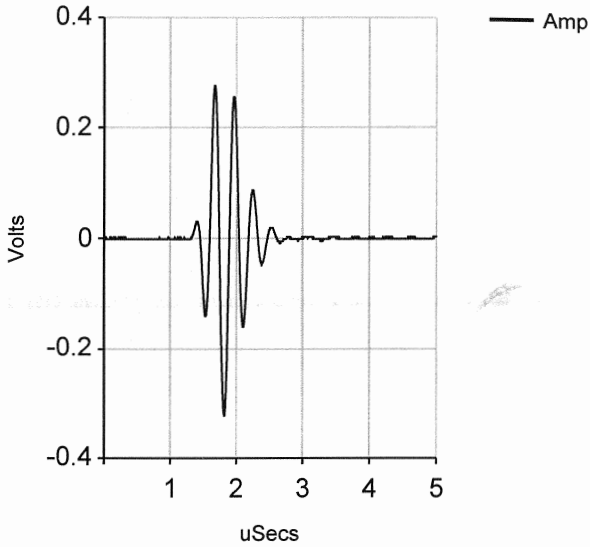

Frequency Spectrum

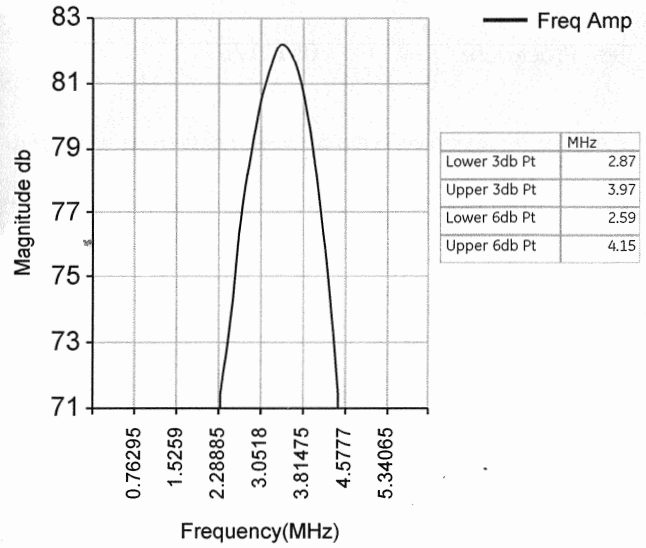

Waveform is first return echo from indicated target.

UTA	Setting
Receiver Imp	50
Pulser Imp	High
Energy	MID-HIGH
Voltage	100
Mode	T/R
Pulser	UTA
HP Filter	1.0 MHz
LP Filter	22.5 MHz
Target	1.0" PLEX GLASS

UTA Gain	19.5
----------	------

Test Data

Test	Min	Measured	Max
Loop Sensitivity(db)	-62	-56.72	-56
Center Freq(MHz)		3.37	
Peak Freq(MHz)	3	3.42	4
6db Bandwidth %	38	46	60
20db Ringdown(usec)		0.944	1.2

UTA SN DA0518  
UTA Cal Due Date 03/28/2019  
O-Scope SN C048089  
O-Scope Cal Date 10/03/2018

Target SN




Transducer Certificate of Conformity  
Compliant to ASTM E-1065

Date	05/21/2018	Serial Number	SAH0023
Part Number	113-223-590	Description	FABP--MSWQC-GAM 3.5X.25
Inspector	AP		
Software	FNT0040	Rev	H
Test Procedure	0511175		

The Ultrasonic Transducer in this document has been performance tested and meets all manufacturing specifications.

The accuracy of the transducer described above has been confirmed by factory standard test equipment and laboratory reference standards traceable to the National Institute of Standards and Technology. This facility's Quality System is registered to ISO 9001-2008 and is compliant to MIL-STD-45662A and ANSINCSL Z540-1-1994.

GE Inspection Technologies, LP  
50 Industrial Park Rd.  
Lewistown, PA 17044

Tel: 717.242.0327  
Fax: 717.242.2606  
GEInspectionTechnologies.com